

Amplitude Response

Kemo Filter Response 41 is a 8 pole Elliptic type filter. Designed with a flat passband, reasonable roll off, and linear phase. A very good general purpose filter, and is available on some Kemo systems with switchable high pass response.

Response 41 Data			
Equivalent Slope		51.8 dB / Octave	
Stopband (theoretical)		> -82 dB	
Overshoot (theoretical)		10.0 % at 1.60 / F_c	
Risetime to 0.996		$1.4/F_c$	
Mean phase line (theoretical)		$-431 f/F_c$	
Attenuation / dB	Normalised Frequency F / F_c		Attenuation / dB
0.10	1.041	1.00	0.0
0.25	1.068	1.10	0.6
0.50	1.095	1.25	5.2
1.00	1.128	1.50	17.5
3.00	1.199	1.75	28.4
6.00	1.268	2	38.1
12.00	1.387	3	83.2
24.00	1.644	4	-
36.00	1.945	5	-
48.00	2.274	8	-
60.00	2.593	10	-
80.00	2.985	-	-


• Kemo Limited

3 Brook Court
Blakeney Road
Beckenham Kent BR3 1HG
www.kemo.com
Tel + 44 (0) 20 8658 3838
Fax + 44 (0) 20 8658 4084

• Kemo Inc.


5 Northbrook Way
Greenville
SC 29615

Tel (864) 297 2522
Fax (864) 675 1530

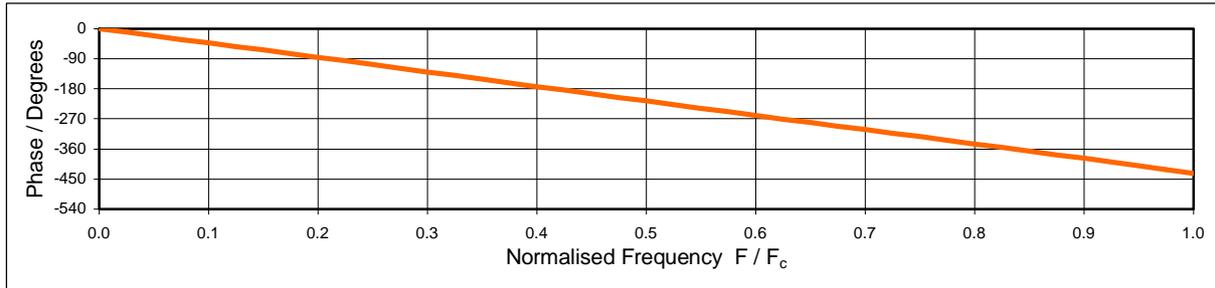


Passband Phase Response

The curve above shows the passband phase response of the Kemo response 41 filter.

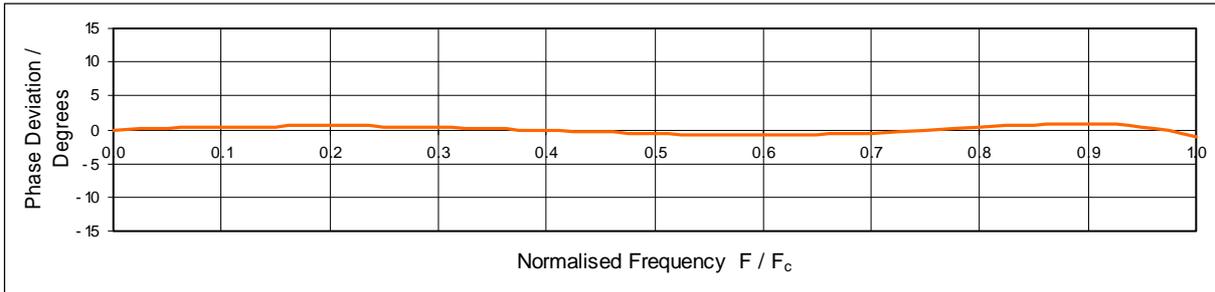

Passband phase deviation

The above curve shows the passband phase variation for the Kemo response 41 filter, this is the difference between the mean phase line and the passband phase response of the filter.

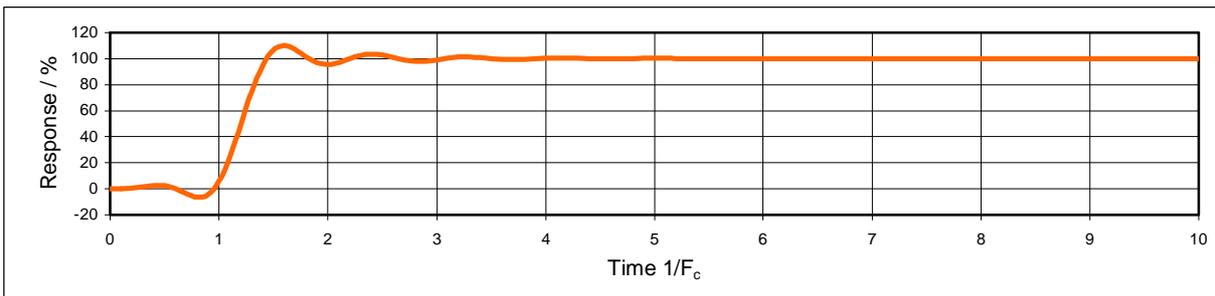

Time Response to Step Input

The curve above shows the time response to a step input to the response 41 filter.

Other Filter Responses

Anti-Aliasing (01) – a filter optimised for anti-aliasing protection before sampling and D-A conversion, where analysis is in the frequency domain.

Butterworth (03) (05) – traditional Butterworth filters, often used to match existing systems, type 01 is superior for alias protection, and type 41 is a better general purpose filter.

Bessel (07) (09) – traditional Bessel filters, linear phase, and small time delay with no overshoot, but significant roll off in the passband.

General Notes about Filter Responses

Selecting a filter is a compromise. We have been manufacturing filters since 1965, and this sheet shows our selection of standard responses built up over a number of years to meet most applications. One of the most important aspects of filter selection is to allow for the total effect on the signal, passband amplitude, phase variation, and step response.

Note- F_c is cut-off frequency

Due to continued product development Kemo Limited reserve the right to change specification without notice

• Kemo Limited

3 Brook Court
Blakeney Road
Beckenham Kent BR3 1HG
www.kemo.com
Tel + 44 (0) 20 8658 3838
Fax + 44 (0) 20 8658 4084

Hochwertige Messtechnik und Beratung aus einer Hand



PCB Synotech GmbH
Porschestra. 20 – 30 ▪ 41836 Hückelhoven
Tel.: +49 (0) 24 33/44 44 40 – 0
E-Mail: info@synotech.de ▪ www.synotech.de

• Kemo Inc.

5 Northbrook Way
Greenville
SC 29615

Tel (864) 297 2522
Fax (864) 675 1530

fr_41.doc